



# LVET0755

## LAB 7.5 HP TRIPLEX VANE VACUUM ENCLOSURE 200G TANK


REVISION NOTES		
DESCRIPTION	ECN	PR/NOR
PRODUCTION RELEASE	PXEC0099	N/A

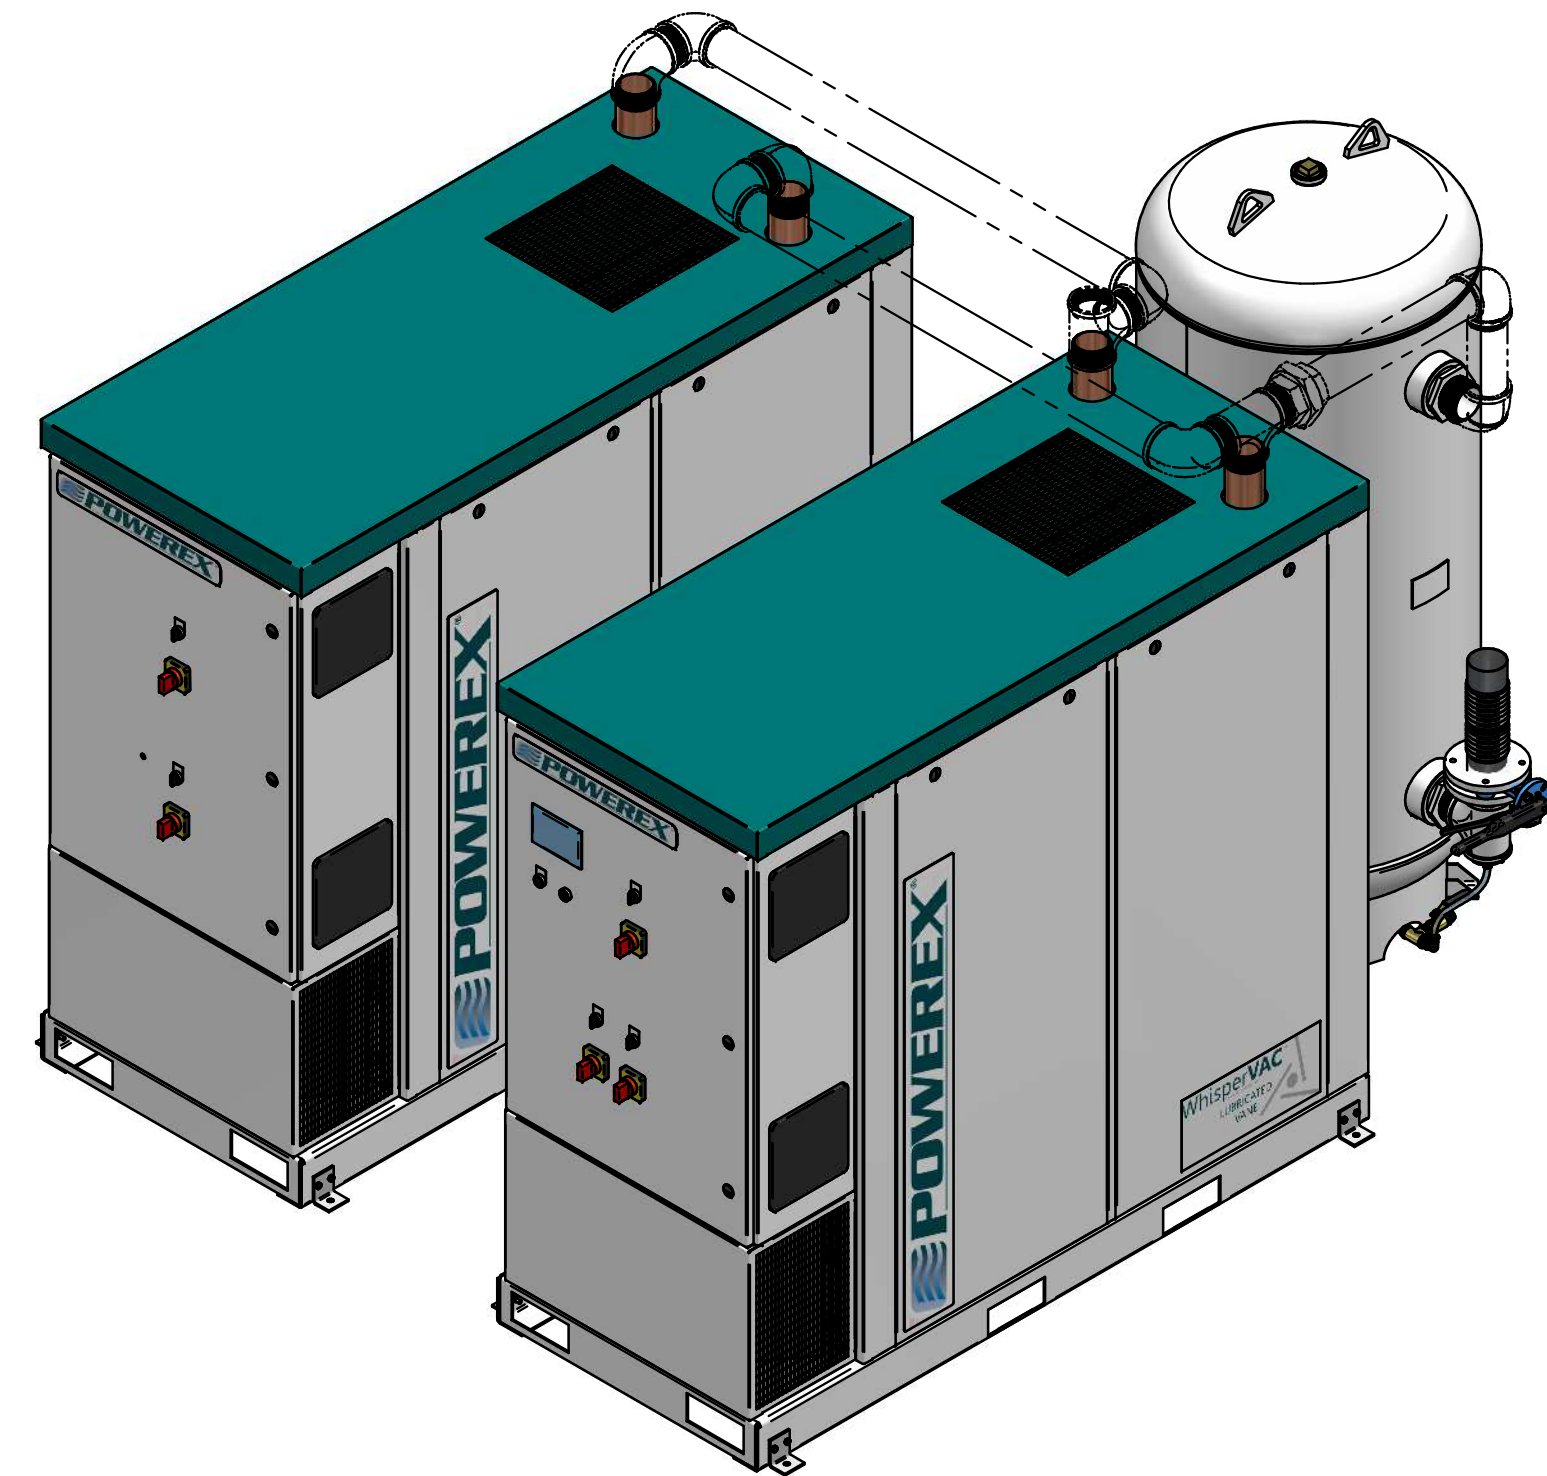


ISO VIEW

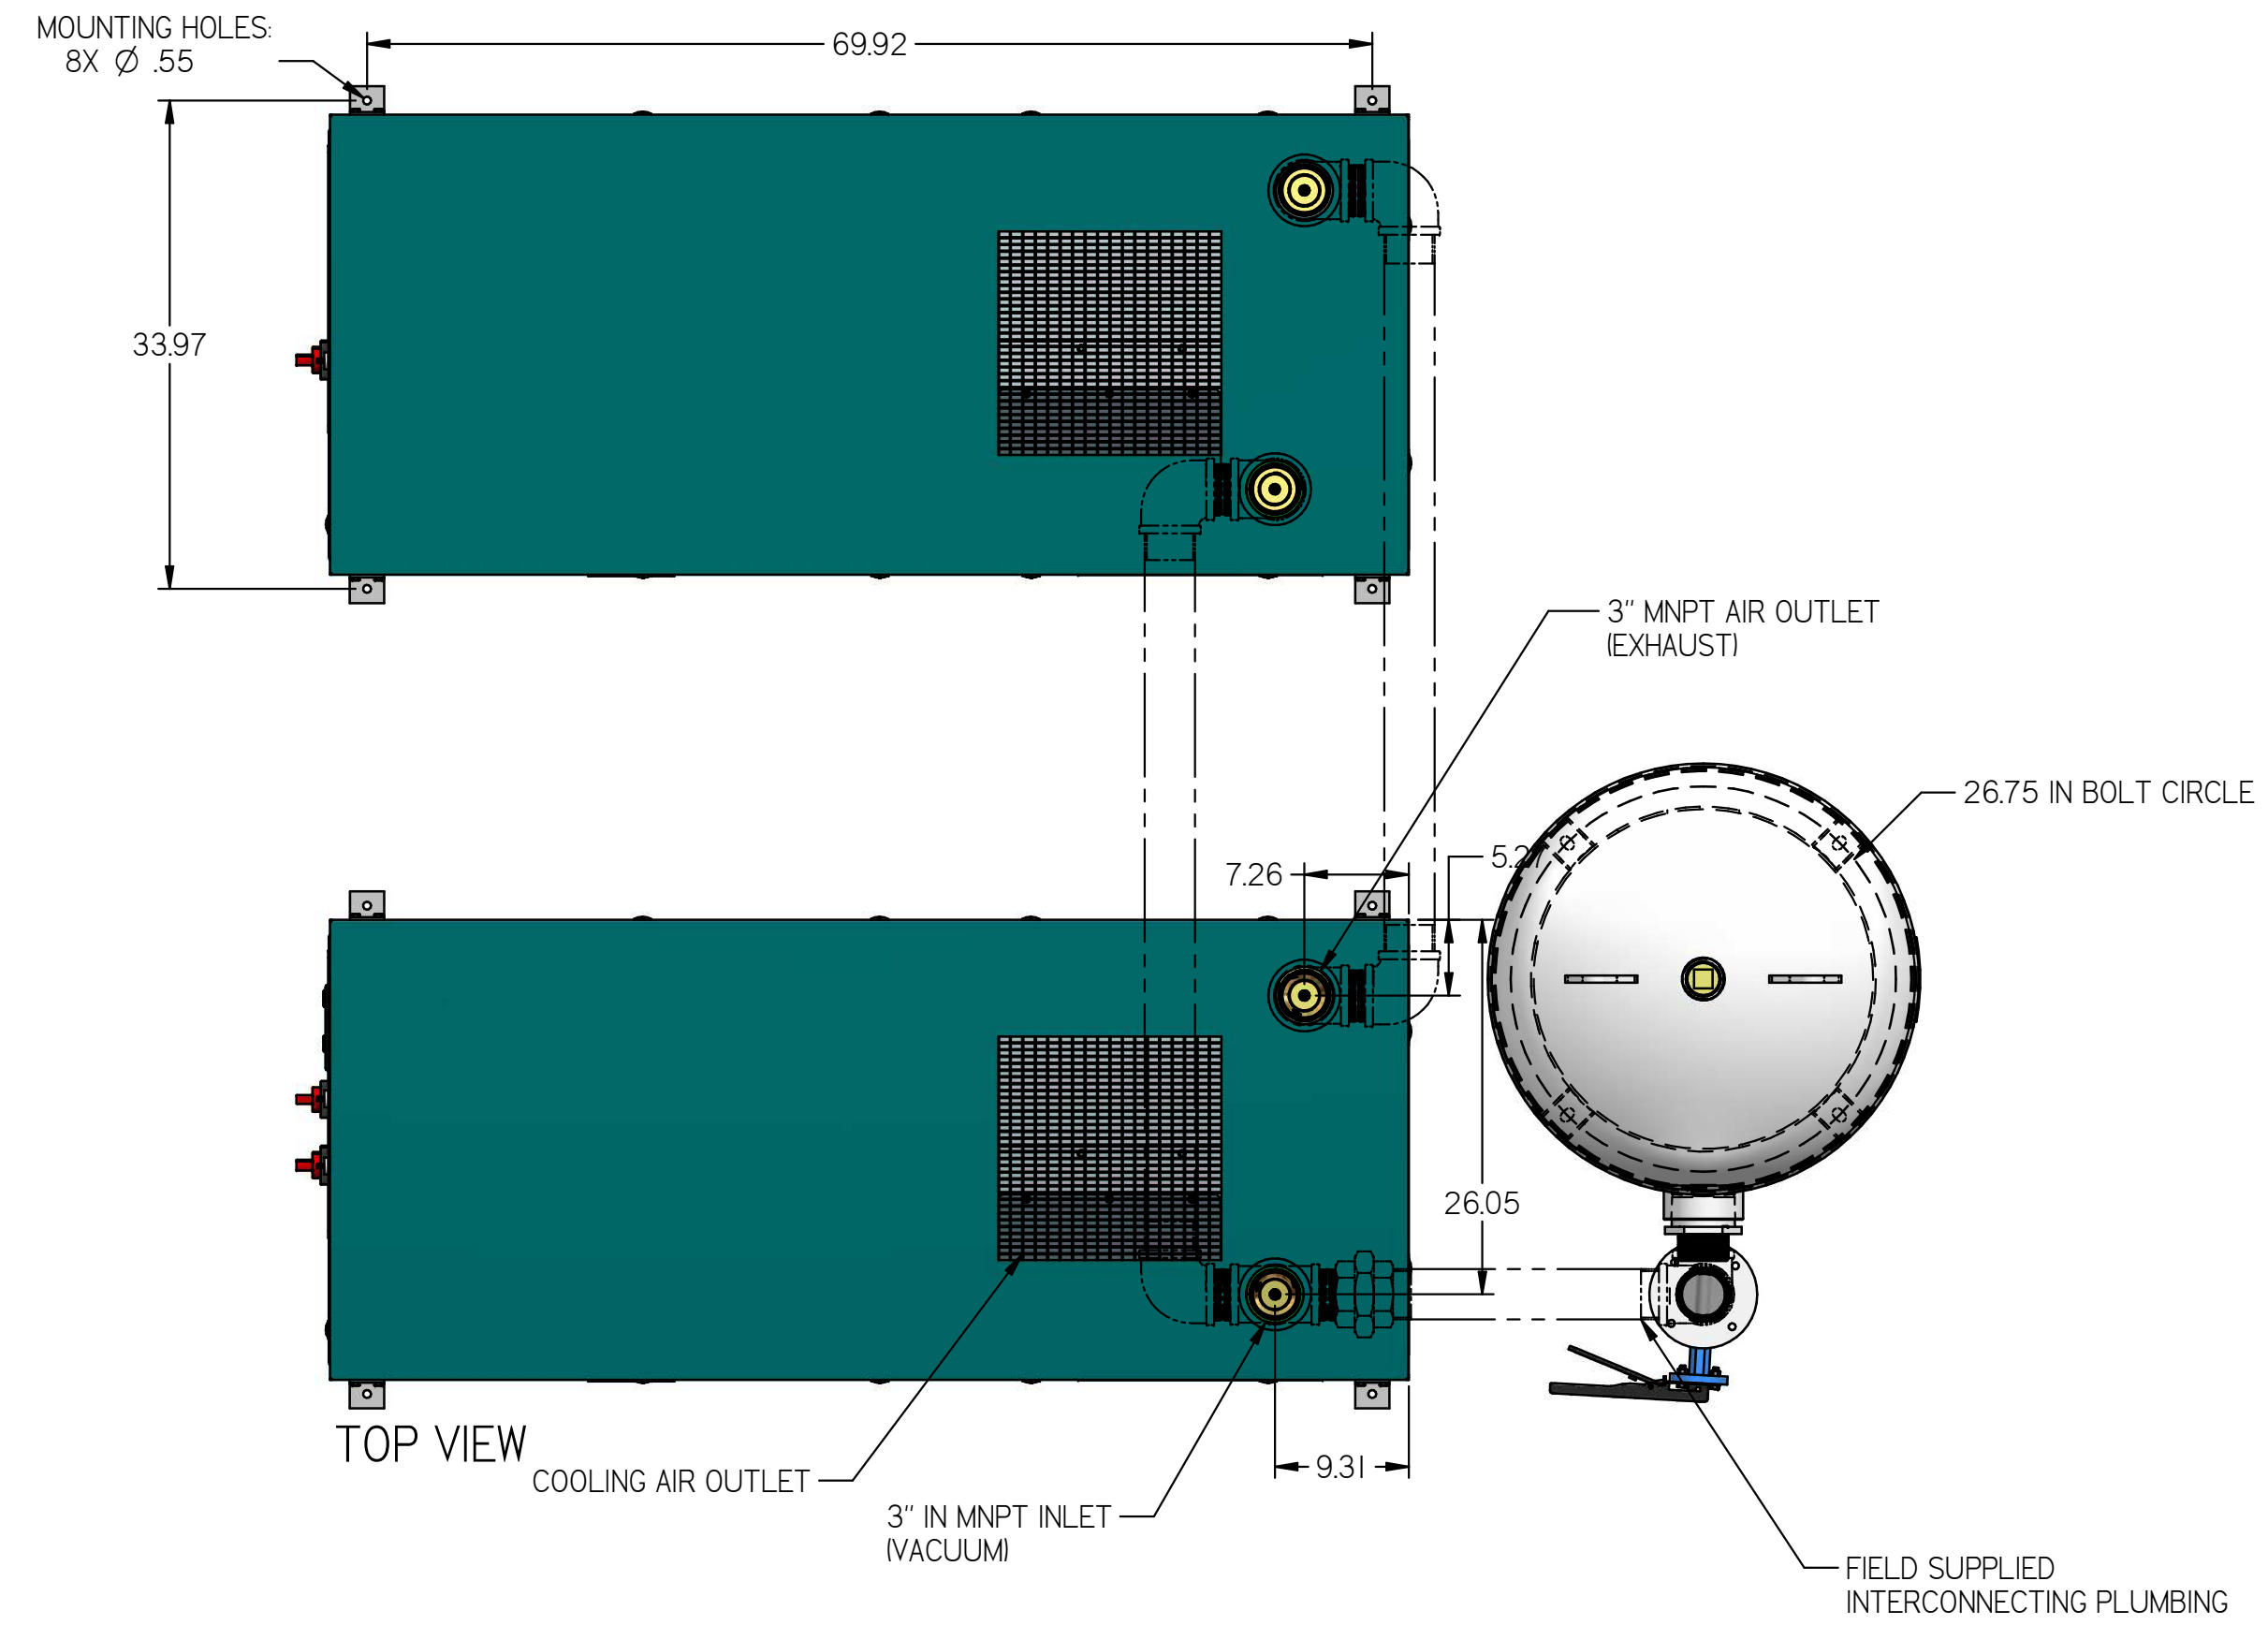

TOP VIEW

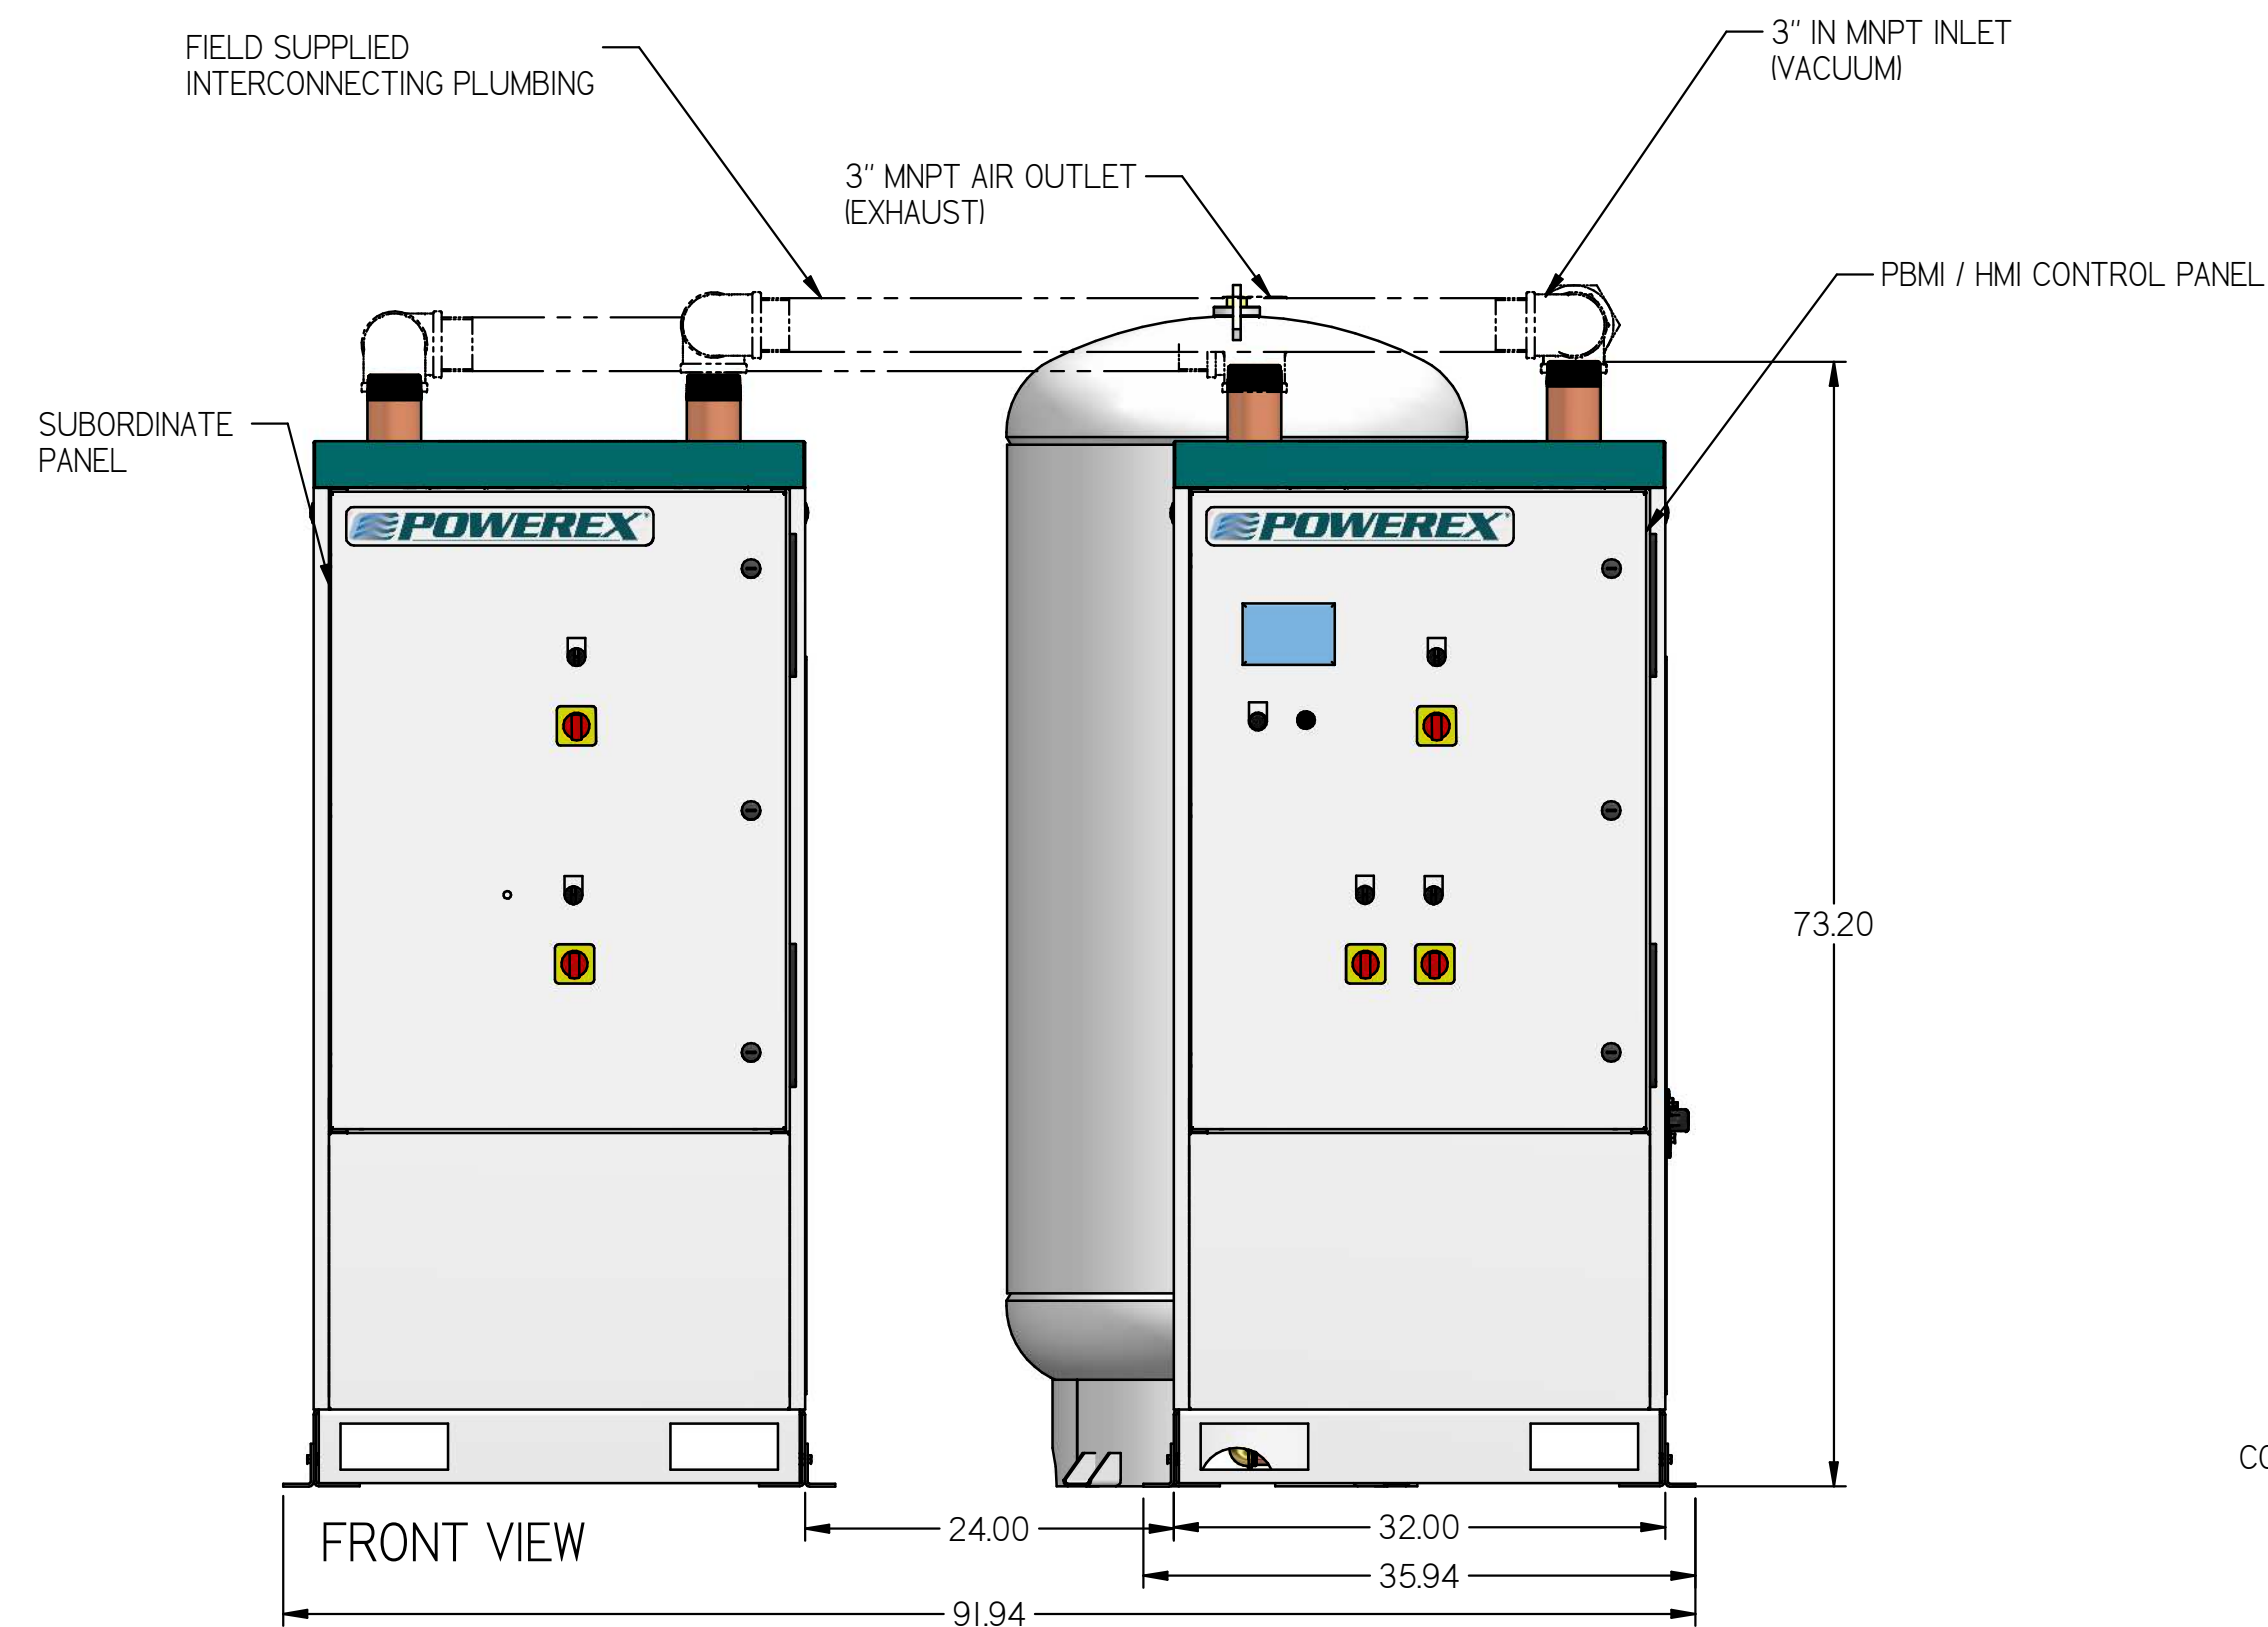

FRONT VIEW

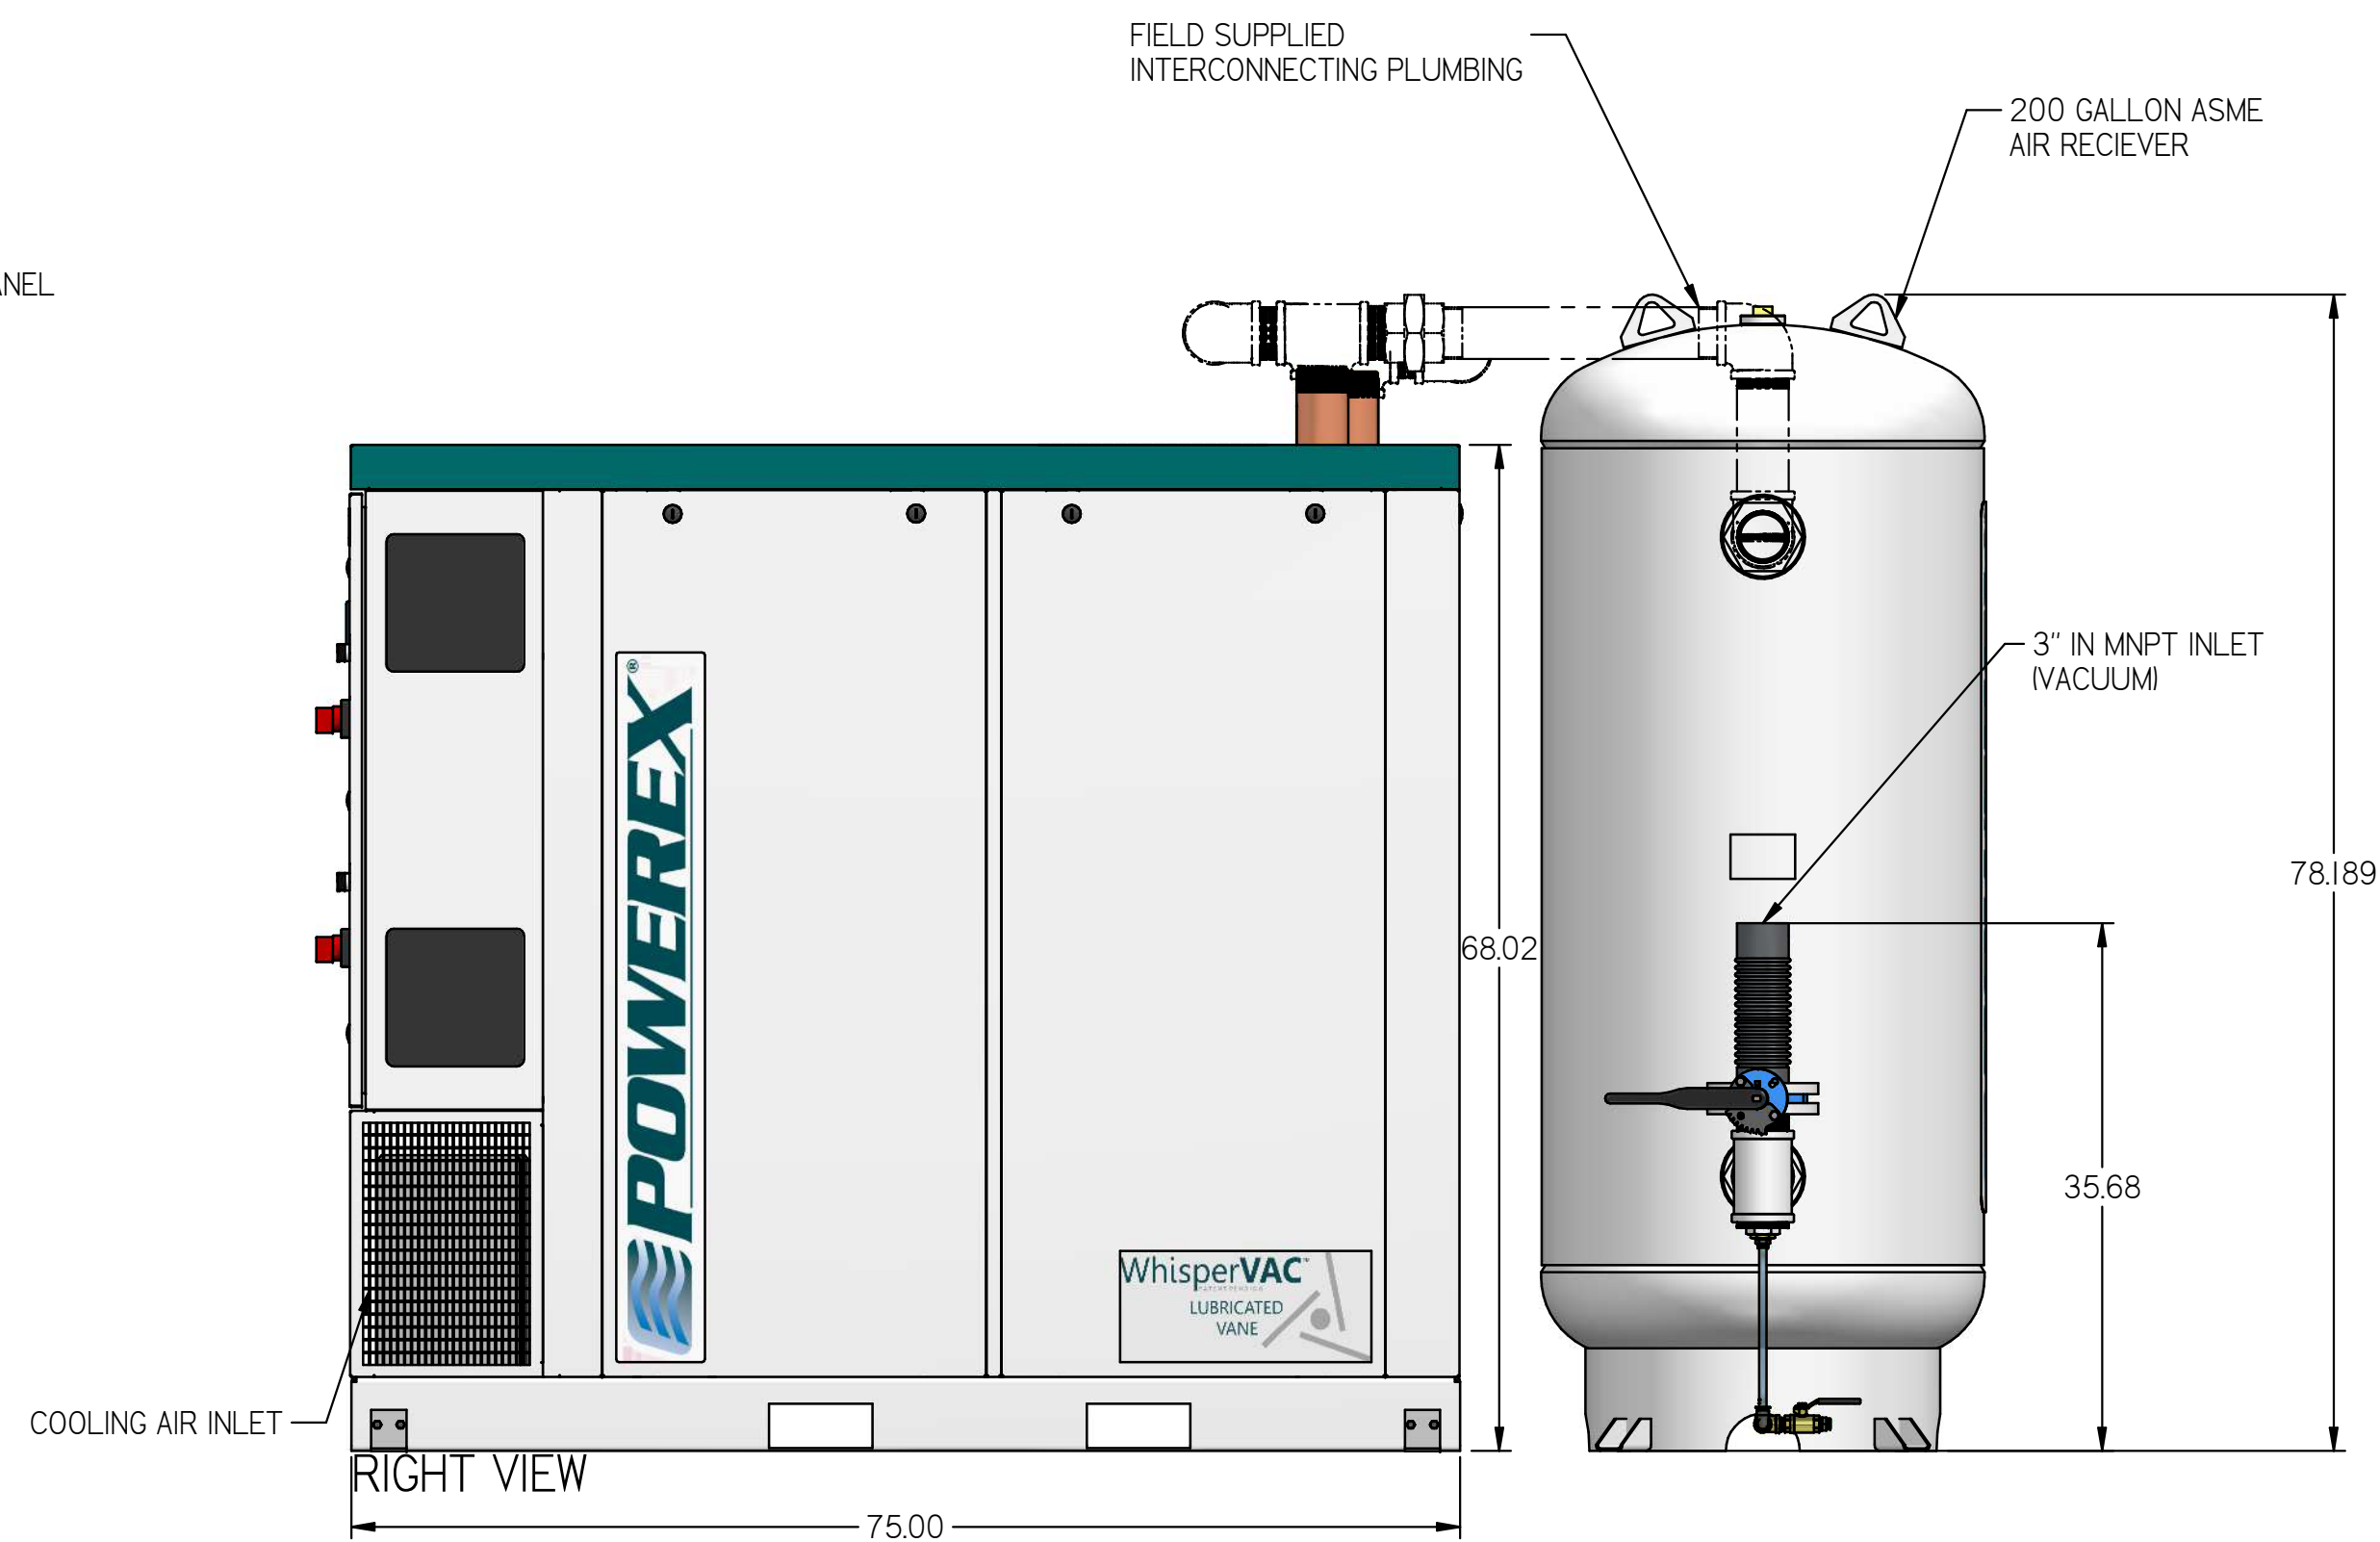

RIGHT VIEW

- NOTES:  
 1. APPROX SYSTEM WEIGHT: 3994 LB  
 2. 24" MINIMUM MAINTENANCE CLEARANCE RECOMMENDED ALL SIDES. CLEARANCE FOR CONTROL PANELS SHALL BE IN ACCORDANCE WITH OSHA/NEC REQUIREMENTS


SYMBOL LEGEND		DRAWINGS TO CONFORM TO CURRENT REVISION OF THE FOLLOWING ANSI STANDARDS: Y14.3 MULTI AND SECTIONAL VIEW DIMS Y14.5 DIMENSIONING AND TOLERANCING	
TOLERANCES NOT SPECIFIED	SOLID EDGE DRAWING	DO NOT SCALE DRAWING FOR DIMENSIONS	
0.00X ± .05	INCH	SHEET 1 OF 2	SCALE 1:1/2.5
0.00X ± .005		APPROVALS ON FILE IN PLM	
CONFIDENTIAL DISCLOSURE This drawing is the property of POWEREX of the SCOTT FETTER COMPANY and is subject to return on demand. Its contents are confidential and must not be copied or submitted to outside parties for use or examination.		AUTHOR	ORIGINATION DATE
TITLE: 717780 MATERIAL: SEE COMPONENT DRAWINGS		ASoulek	2/7/2019
DESCRIPTION: LAB 7.5 HP TRIPLEX VANE VACUUM ENCLOSURE 200G TANK		DRAWING NUMBER: LVET0755	
		REVISION	SIZE
		B	D



# LVET0755

## LAB 7.5 HP TRIPLEX VANE VACUUM ENCLOSURE 200G TANK

REVISION NOTES		
DESCRIPTION	ECN	PR/NOR
PRODUCTION RELEASE	PXEC0099	N/A

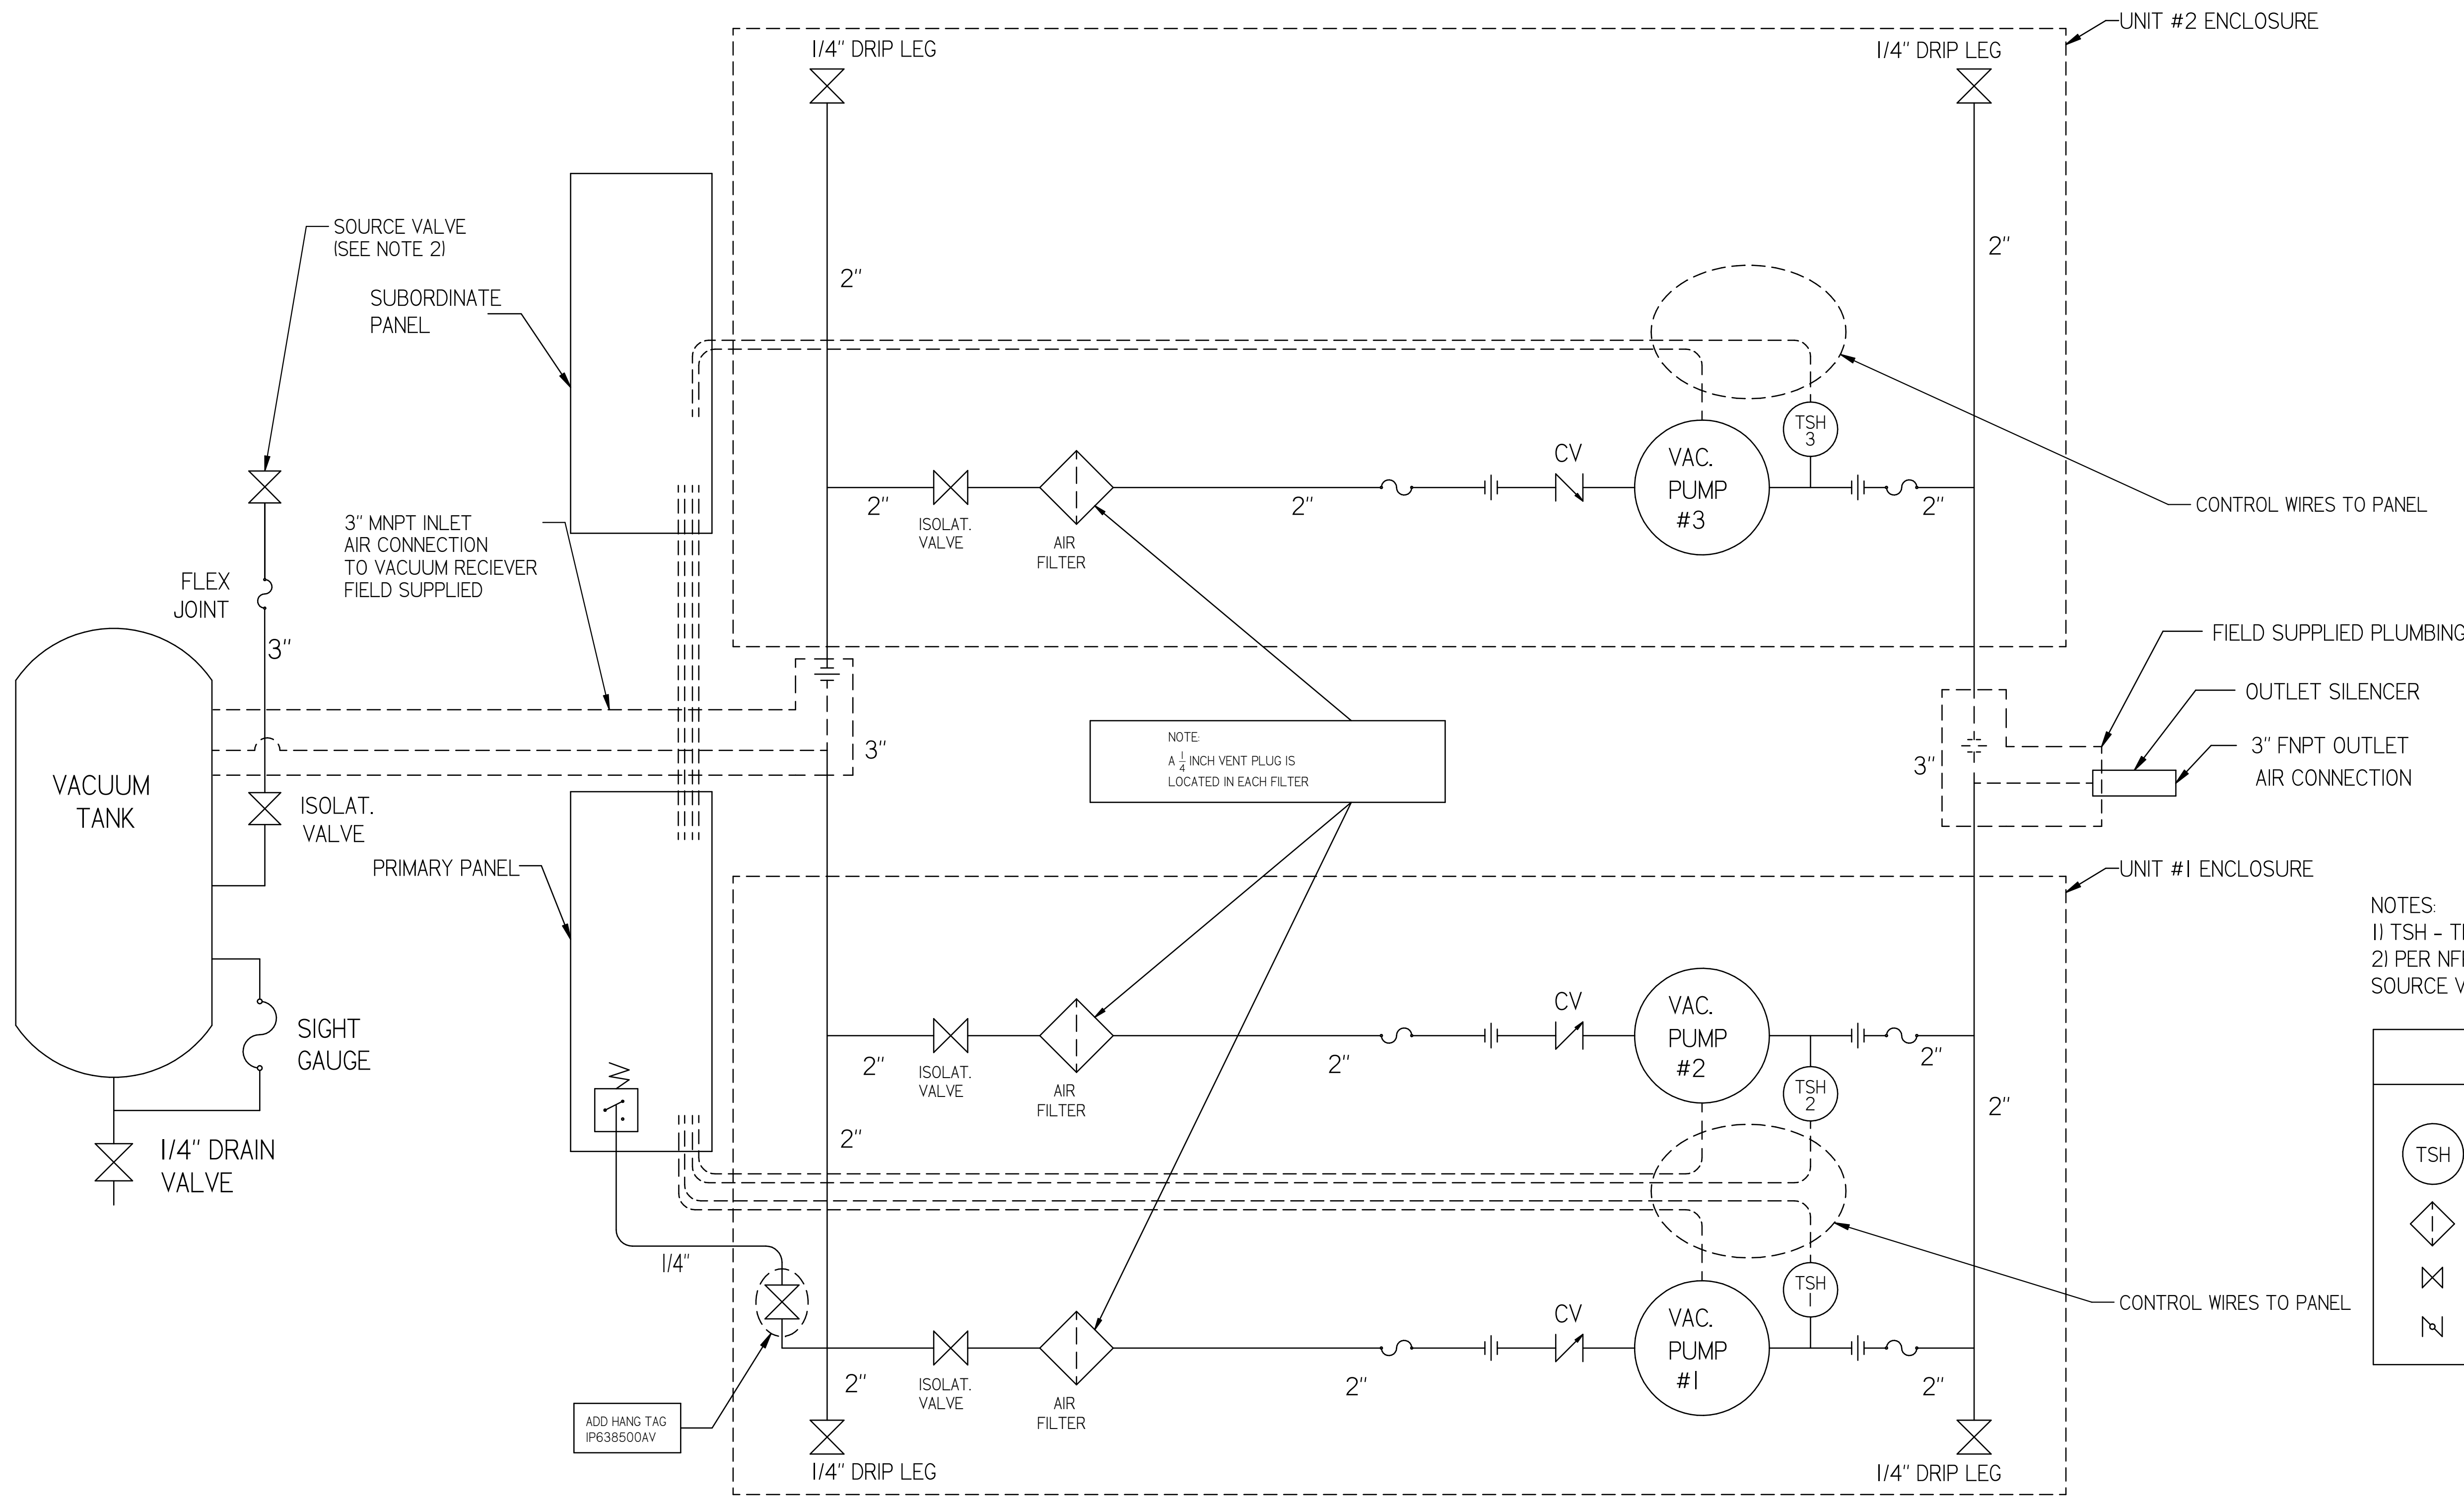

NOTE:  
A 1/2" INCH VENT PLUG IS  
LOCATED IN EACH FILTER

- NOTES:  
1) TSH - TEMPERATURE SWITCH HIGH  
2) PER NFPA THE SYSTEM WILL REQUIRE A  
SOURCE VALVE (SUPPLIED BY OTHERS).

LEGEND	
(TSH)	TEMP. SWITCH
◇	AIR FILTER
⊗	BALL VALVE
⌞	BUTTERFLY BALL VALVE
⊞	VACUUM TRANSDUCER
⌞	CHECK VALVE
~	FLEX LINE
-	UNION

SYMBOL LEGEND	DRAWINGS TO CONFORM TO CURRENT REVISION OF THE FOLLOWING ANSI STANDARDS: #14.3 MULTI AND SECTIONAL VIEW DIMS #14.5 DIMENSIONING AND TOLERANCING		
TOLERANCES NOT SPECIFIED	SOLID EDGE DRAWING	DO NOT SCALE DRAWING FOR DIMENSIONS	
0.0XX ± .05	INCH	SHEET 2 OF 2	SCALE 1:1
0.0XX ± .005	INCH	APPROVALS ON FILE IN PLM	
<small>CONFIDENTIAL DISCLOSURE</small> <small>This drawing is the property of POMEREX of the SCOTT FETTER COMPANY and is subject to return on demand. Its contents are confidential and must not be copied or submitted to outside parties for use or examination.</small>		AUTHOR	ORIGINATION DATE
<small>CONFIDENTIAL DISCLOSURE</small> <small>This drawing is the property of POMEREX of the SCOTT FETTER COMPANY and is subject to return on demand. Its contents are confidential and must not be copied or submitted to outside parties for use or examination.</small>		ASoulek	2/7/2019
ITEM NO: 717780			
MATERIAL: SEE COMPONENT DRAWINGS	<small>150 PRODUCTION DRIVE, HARRISON OH 45030</small> <small>888.768.7079</small>		
DESCRIPTION: LAB 7.5 HP TRIPLEX VANE VACUUM ENCLOSURE 200G TANK	DRAWING NUMBER: LVET0755	REVISION: B	SIZE: D